

---

# Product instruction

Product model:TR-OPC04 Beauty Bed

## Product overview


Product model	TR-OPC04 beauty bed
Back of a chair size	58 cm *65cm
The cushion size	50cm*65cm
The leg size	60cm *65cm
Lifting height	Min: 62 cm Max: 85 cm
Packing size	165 cm * 65cm * 65cm
Package number	1 piece/carton
The main body material	High density sponge, metal support, etc
The weight of the	85kgs
The largest bearing	150kg
color	White black <input type="checkbox"/> lake blue <input type="checkbox"/> ⚙
Product characteristics	1. High performance mute motor (110/220V) controls the overall lifting
	2. Adjustable middle seat tilt, suitable for different sitting position and sleeping position
	3. The overall elevation of the head and legs can be adjusted separately
	4. Motor CE,TUV certification, appearance patent certificate
Optional configuration	Drag three drag four side control (with foot control) <input type="checkbox"/> casters <input type="checkbox"/> ● ⚙

Beauty bed is widely used in beauty salon, body massage club, SPA, micro plastic surgery medical industry, tattoo tattoo chain.The operation is simple and convenient, safe and stable, and its unique structure design

---

contributes to the various angles and directions of the body in the process of beauty and beauty, which is convenient for beauticians to carry out corresponding nursing operations.

## 1.Product structure drawing:

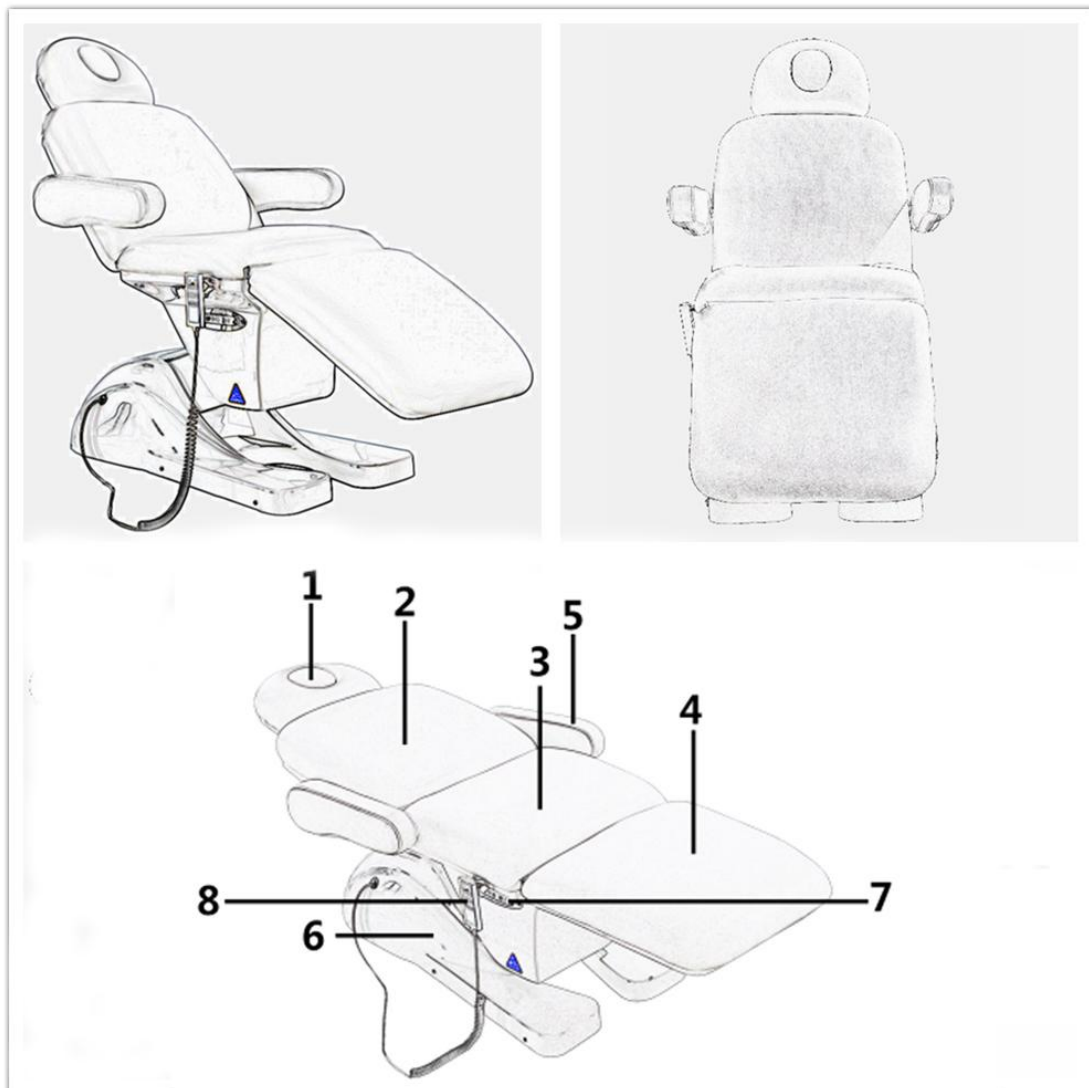

- ①Headrest
- ②Backrest
- ③Cushion
- ④Foot pad
- ⑤Armrest
- ⑥ABS blister cover
- ⑦USB connection and power socket

---

## ⑧ Remote control box

### 2. Product instructions

Beauty bed is shipped in one piece, so after the user puts the beauty bed, plug in the power cord (three-phase 220V/110V) and the remote control cord, and it can be used.

The beauty bed standard is equipped with three motor control (if the optional hand control and foot control need to add a controller), control the overall rise and fall, hand control seat Angle to meet the beauty of the body in the process of various angles, orientation of the body. Adding foot control is the preferred configuration during aseptic operation! The pillow has an air vent, which accords with the aesthetic design of human body. The armrest on the side of cosmetic bed is divided into two parts. The way to install armrest is to adjust the back of the bed to stand up first, and then insert the armrest into the appropriate position with the card slot. Handrails can be disassembled according to the demand for convenience, or temporarily adjusted directly to put back. The head can be adjusted to meet different nursing requirements by manually adjusting the automatic clamping position of the plunger.

---

### 3.Matters needing attention

- ◆ The access voltage of the product must be three-phase 220V/110V, the lack of meeting will cause power safety hazards;
- ◆ The base bracket adopts the hardware bracket structure, which should not be moved or put violently when handling and placing, and should not be hit or smashed with hard objects, so as to avoid damaging the metal bracket structure of the base and affecting the product experience.
- ◆ Whenever customers want to prepare for the top seat, should be remote control in advance to operate the bed body into a chair state, the back of the armrest does not block customers, because the main force of the bed in the middle seat, customers must be in the middle seat up and down, in order to longer service life of the bed body, it is prohibited in the legs up and down on the back.
- ◆ The pillows, backrests, seat cushions, legs, and left and right armrests are all made of high-quality leather, so avoid contact with hard objects or sharp objects when placing them, so as not to damage the leather;

- 
- ◆ The remote control should be put back on the hook after each use. It should not be misplaced to avoid trampling on the remote control while walking.

#### 4. Maintenance instructions

- ◆ This product should be placed in a ventilated and dry environment with appropriate temperature. It should not be placed in a high temperature or humid place.
- ◆ After each nursing operation, to clean the beauty bed body, to ensure the use of health;
- ◆ The base ABS blister is attached with a protective film before delivery to ensure the quality of the product;When you go back to use, tear off the protective film can be as good as new.
- ◆ When there are stains on the surface, please use professional cleaning fluid to clean;

---

## 5. After-sales description

Thank you very much for your trust, choose our beauty bed products, division I is a collection of research and development, production, sales of beauty medical tattoo equipment in one of the high-tech enterprises.

We pay special attention to technology research and new product development. Our research and development team focuses on how to rationalize product structure and standardize production, and engineers enhance the added value of products through innovative product design, structural design and manufacturing processes. At present, our products or key components have been approved invention patents, utility model patents, appearance patents.

Our company has a quality control team composed of several professional quality inspection engineers, who strictly control the quality of products. From the purchase of raw materials to each production process, our company carries out strict management according to ISO 9001 quality system.

If you have any questions in the future use process, you can contact our customer service, will serve you wholeheartedly!

---

## 6. Instructions on aftersales and warranty

The whole structure of the product is guaranteed for one year, and the special motor for the electric bed is guaranteed for three years.

---